

FIG. 1

2/5
JOSE ARNO
ATMI-567

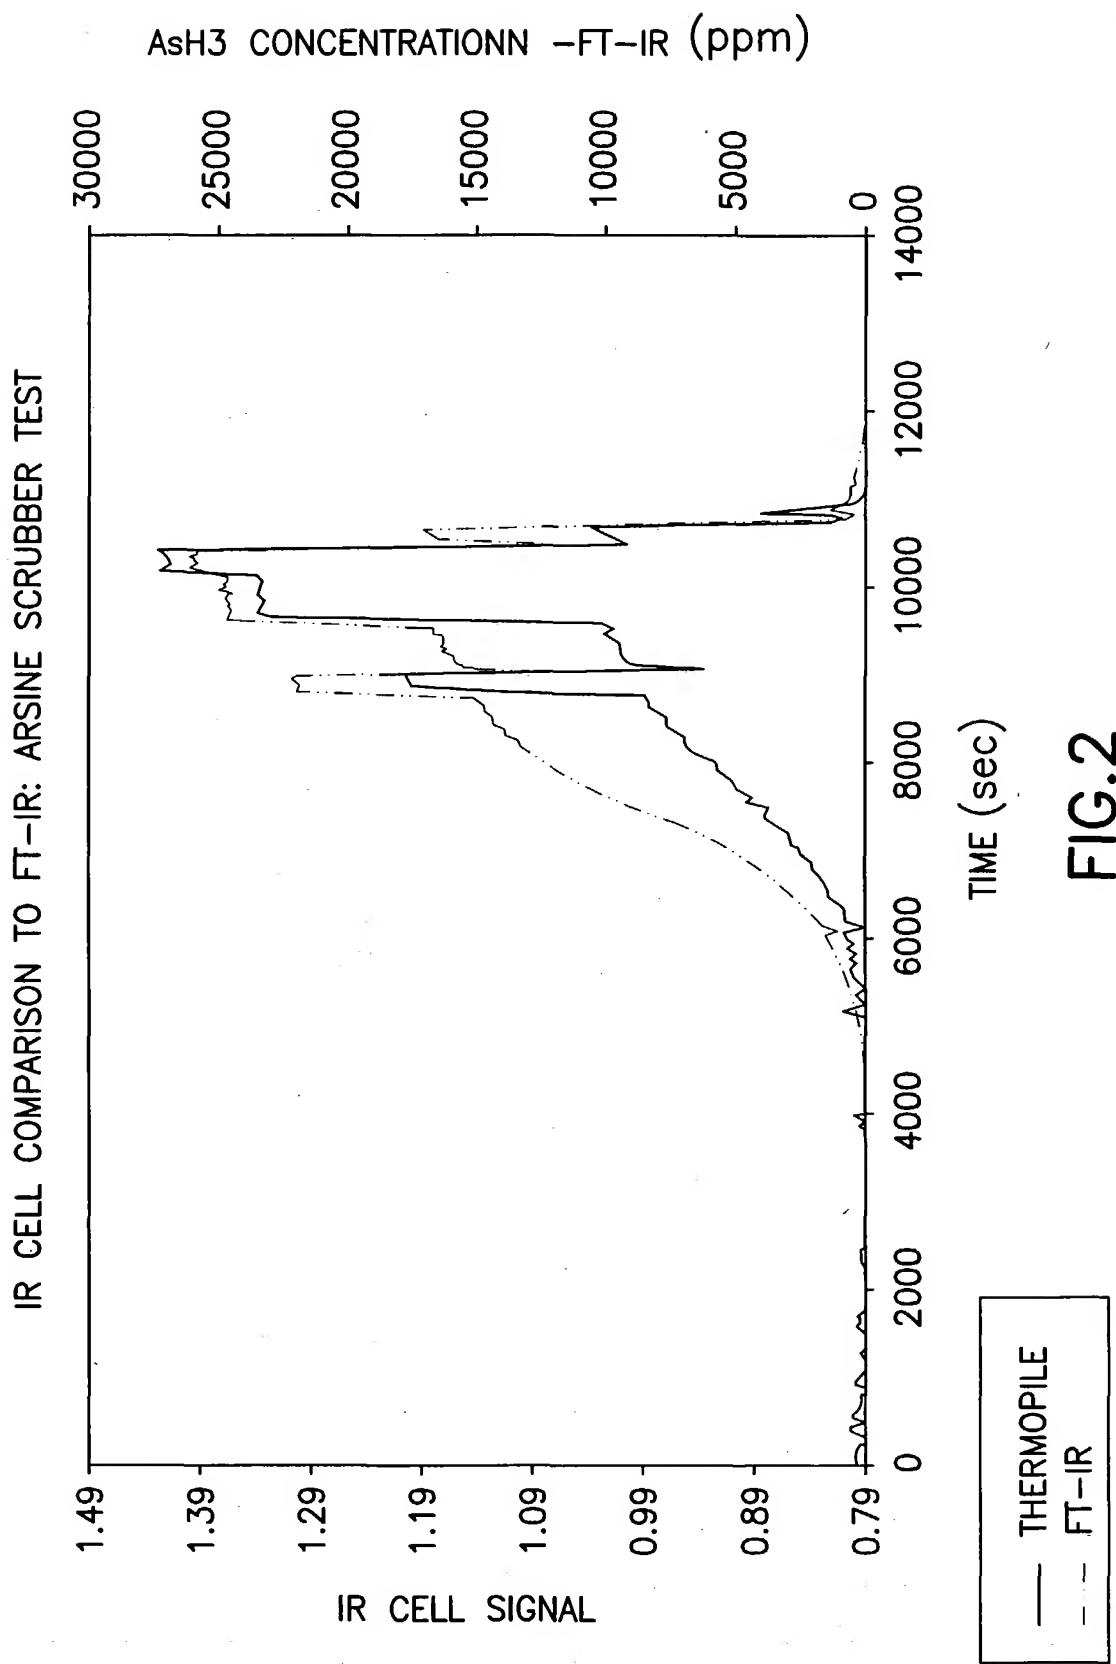


FIG.2


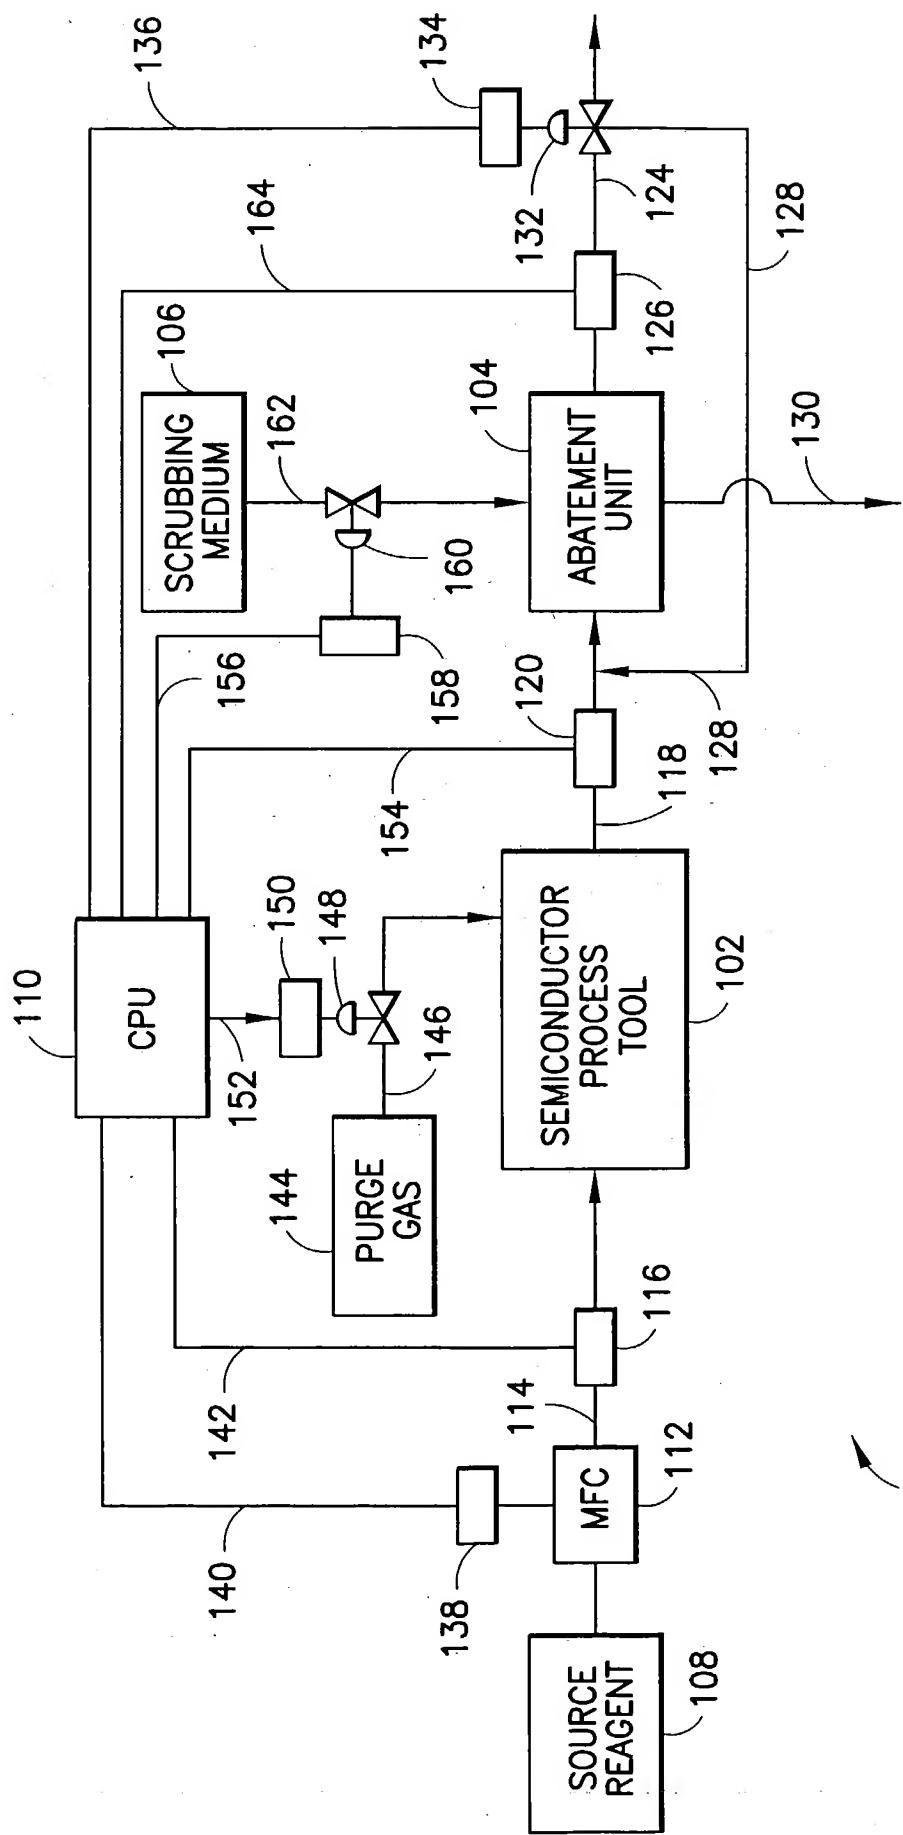


FIG. 3

TIME DEPENDENT RESPONSE OF TP MONITOR WITH CHANGING
3MS CONCENTRATIONS

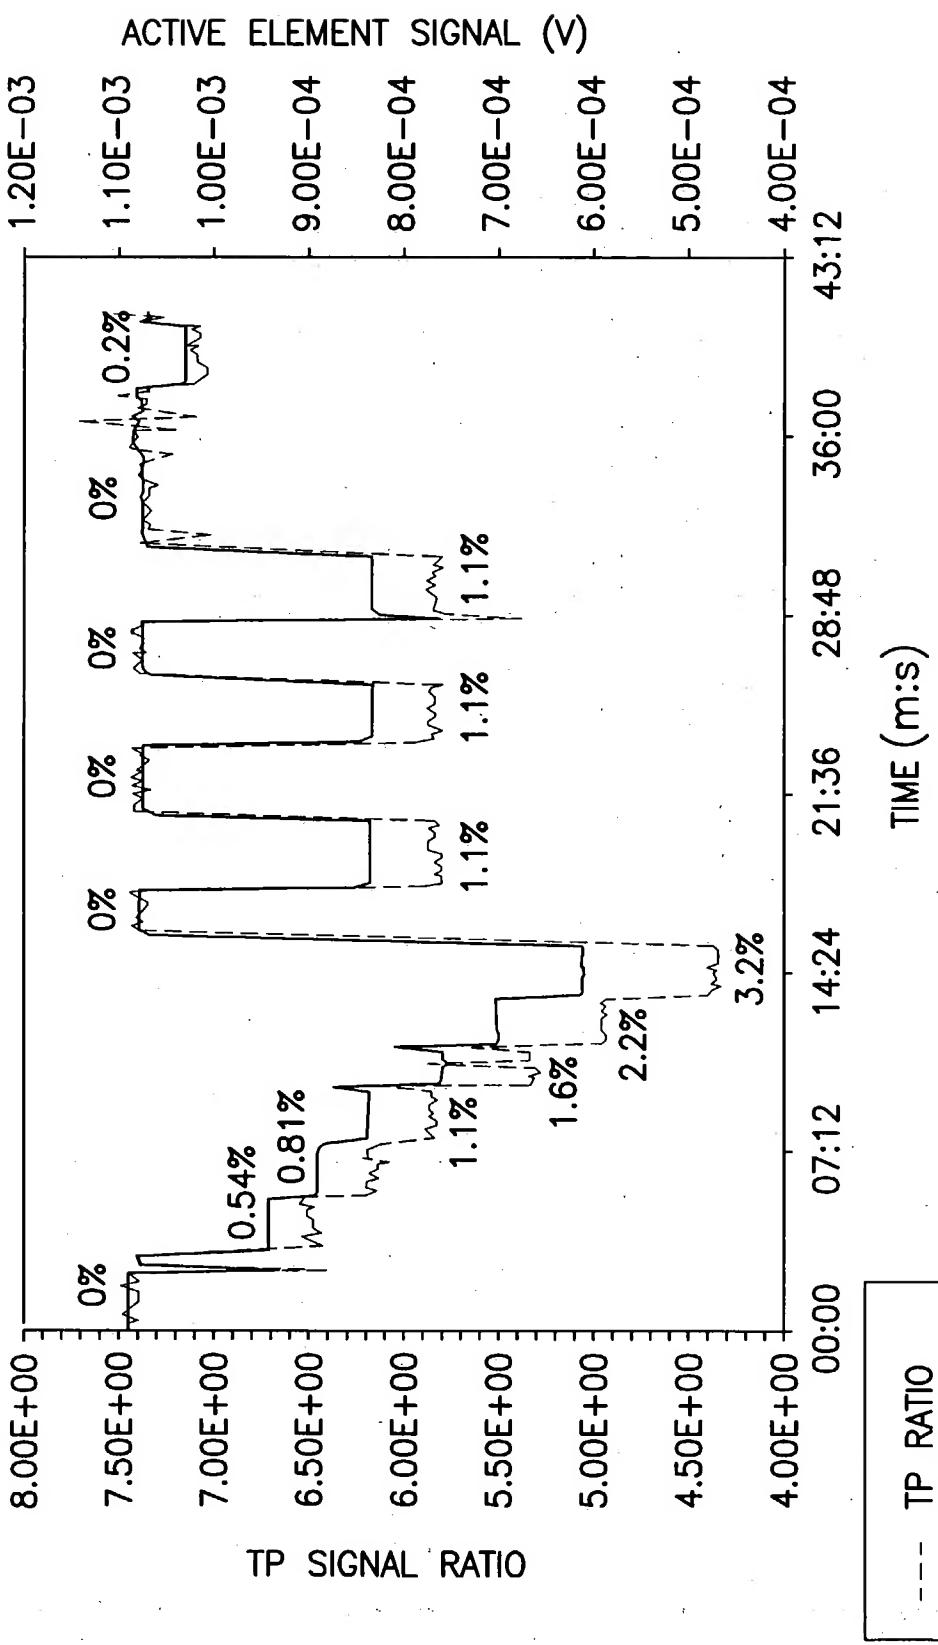

% NUMBERS CORRESPOND TO
3MS CONCENTRATION

FIG. 4

THERMOPILE SYSTEM CALIBRATION USING
3MS (10 cm PATHLENGTH)

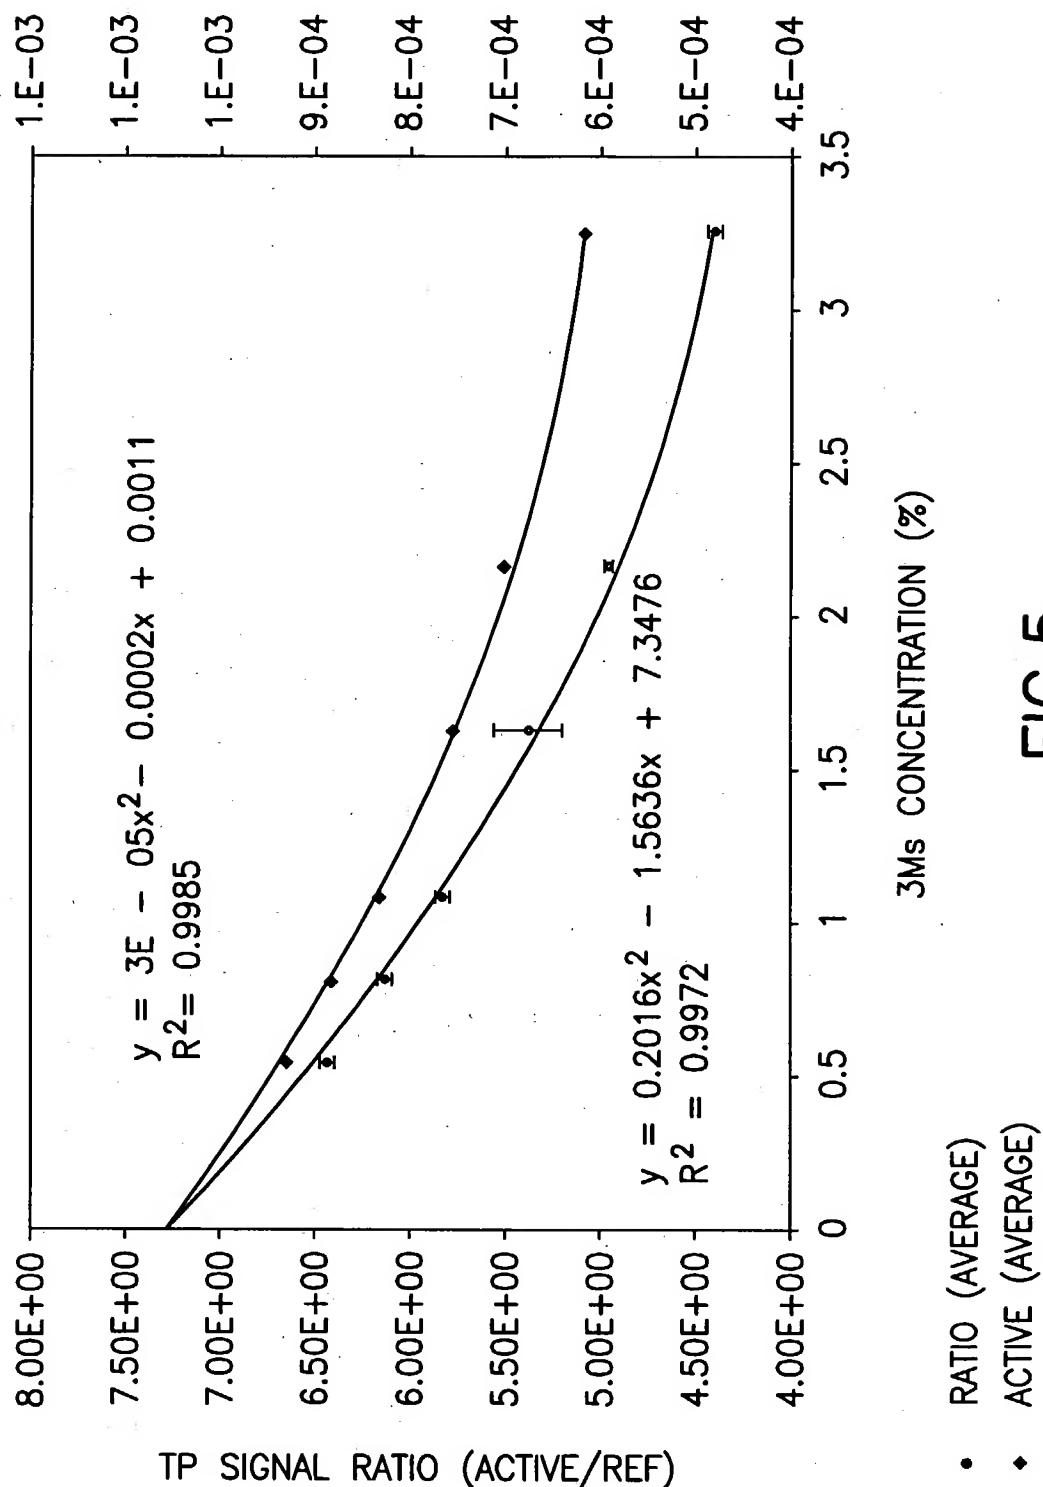


FIG. 5